

# Calibration of the Vertical Cavity Surface Emitting Laser (VCSEL) water vapor hydrometer



Minghui Diao

Department of Meteorology and Climate Science


San Jose State University

SOCRATES science meeting  
November 27, 2018




# Outline

- 1. Laboratory calibration set-up
- 2. Calibration result
- 3. Application to the SOCRATES water vapor data
- 4. Relative humidity frequency distribution
- 5. Summary and future work

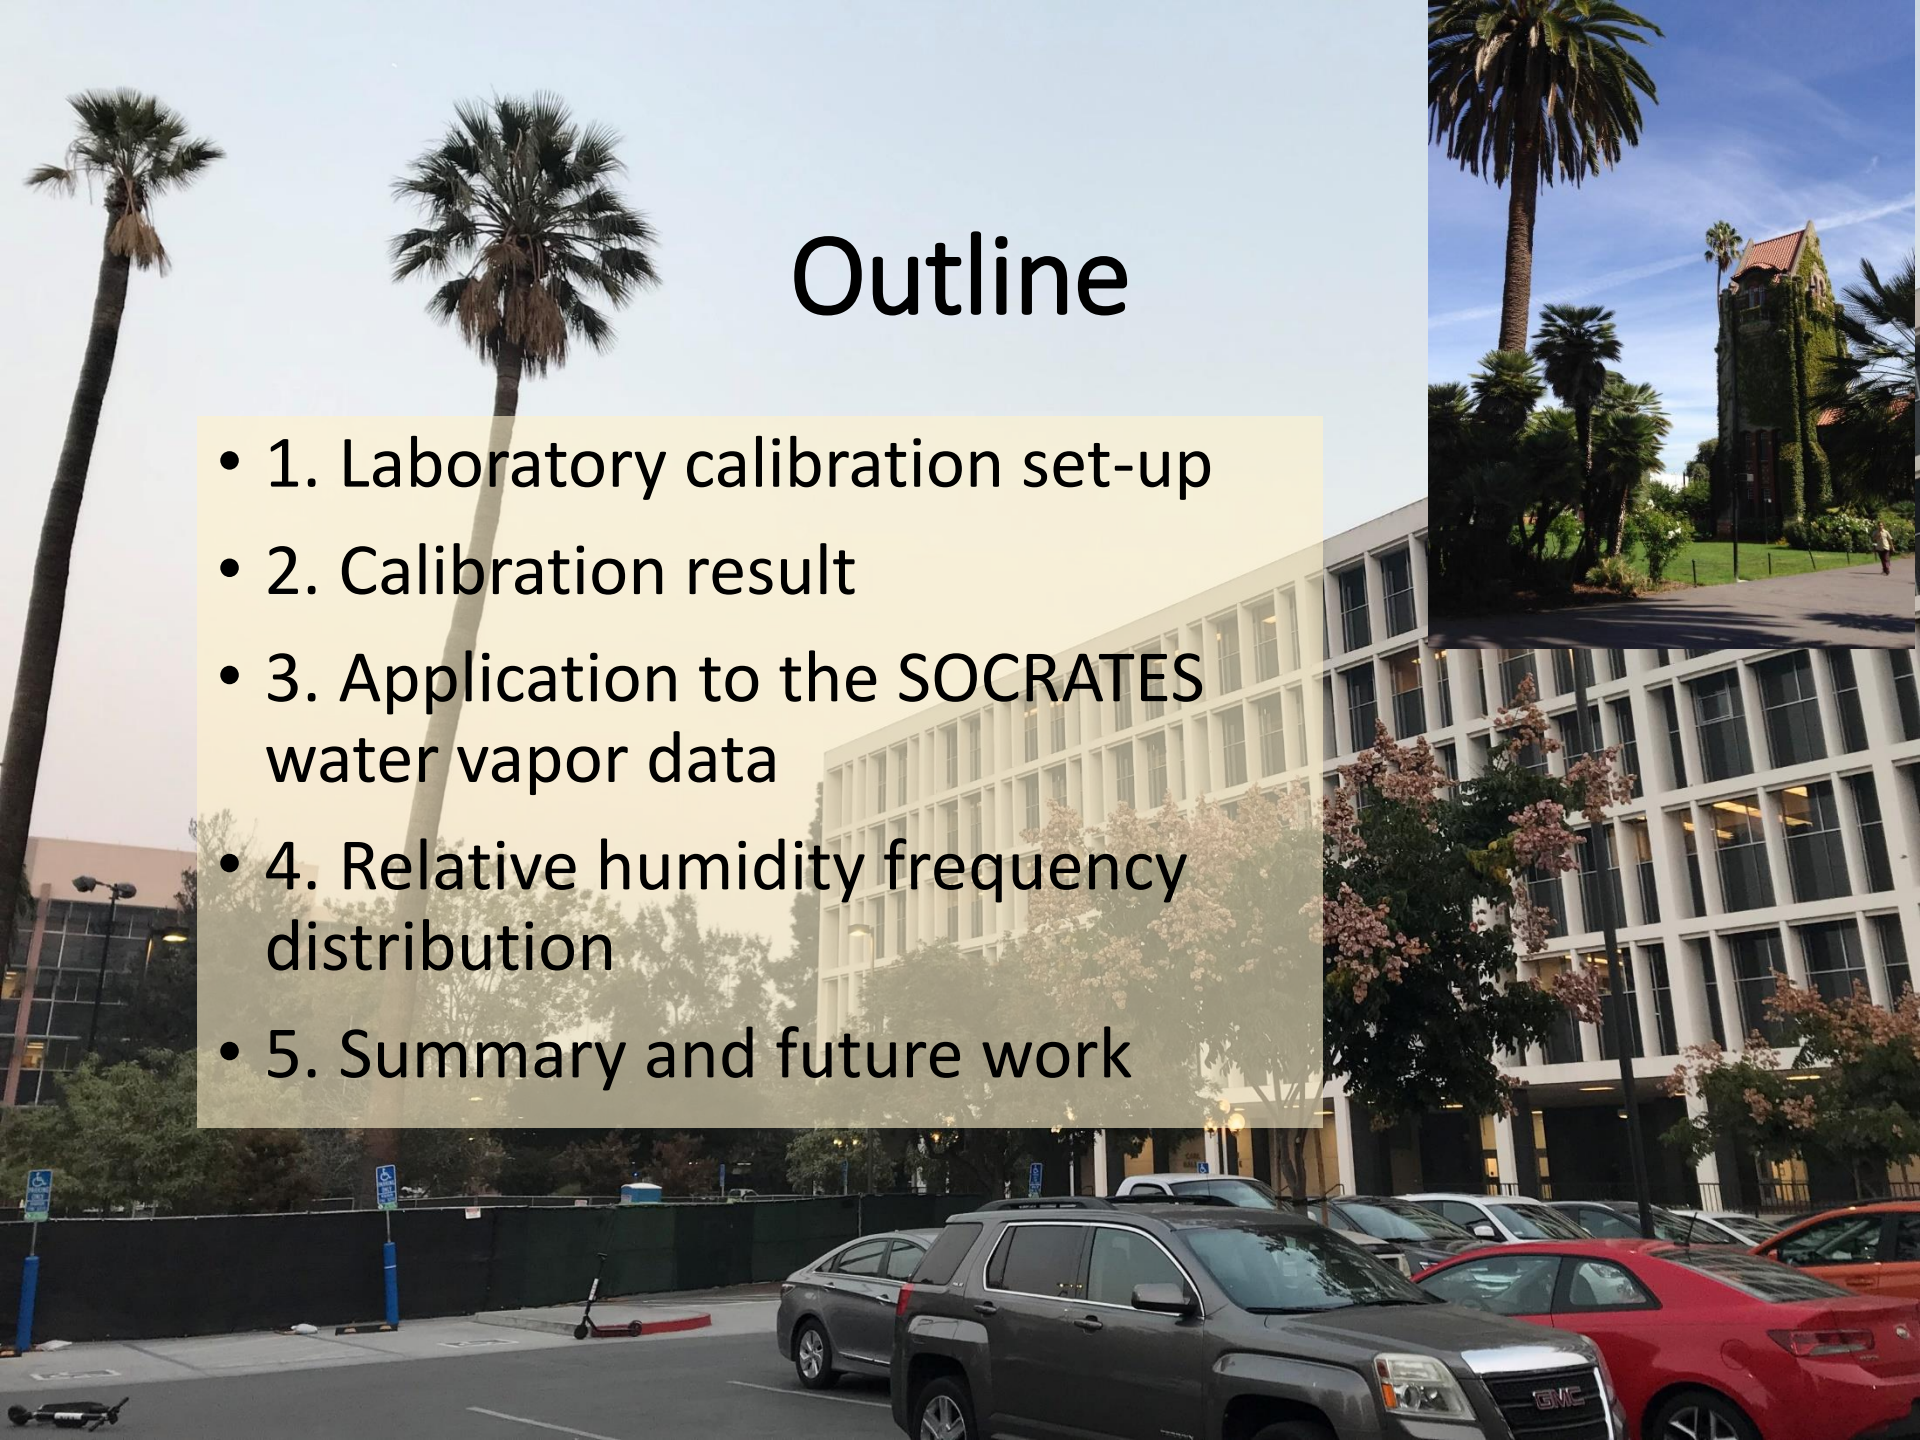

# Laboratory experiment design

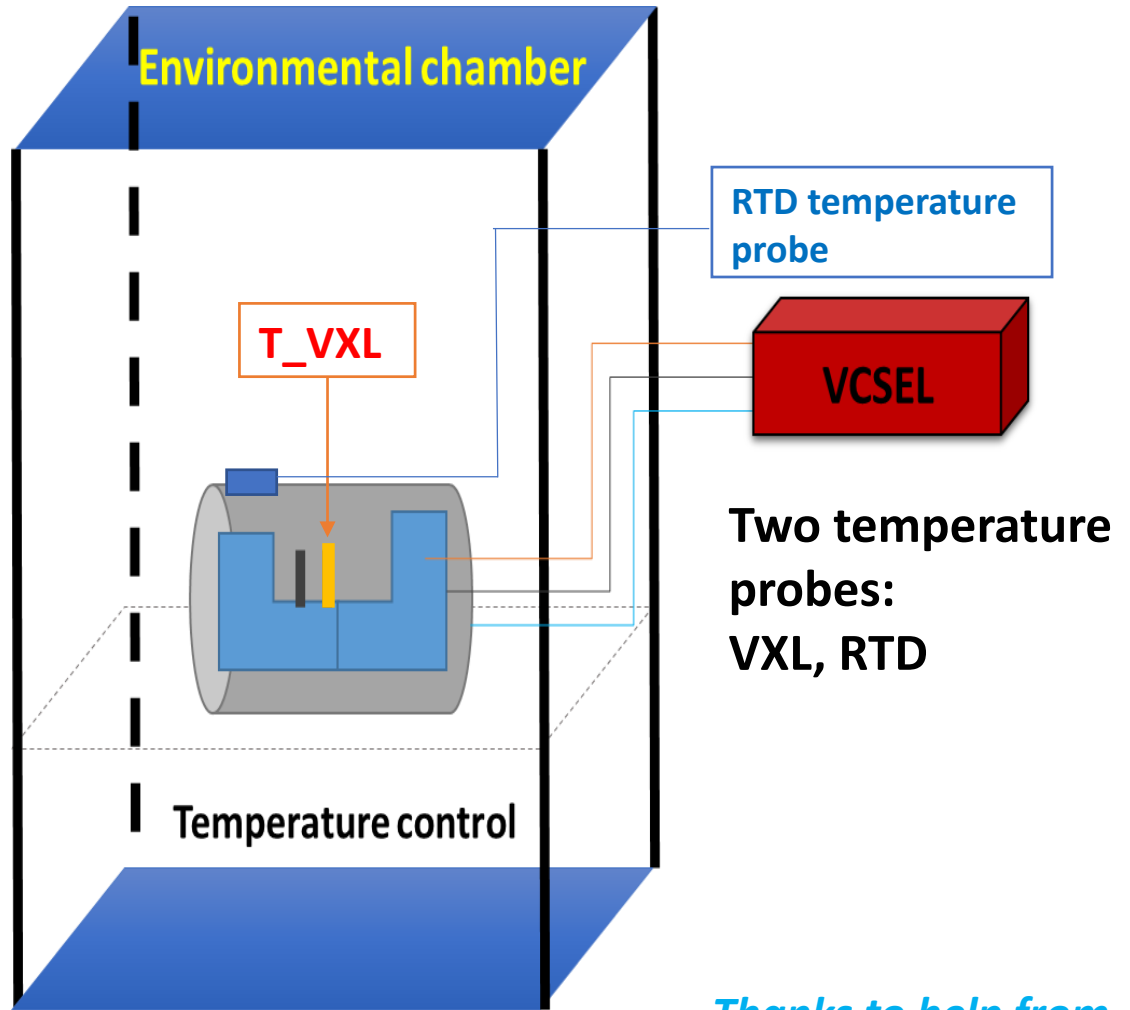

## Fundamental physics:

Saturation vapor pressure ( $e_s$ ) is determined by temperature only

$e_{s_{ice}}$  and  $e_{s_{liq}}$  are calculated based on Murphy and Koop (2005)

*Thanks to help from Stuart Beaton, Laura Tudor and Hendrik Gilmer*

# Evaluation of the calibration system



## 1. Does temperature series vary when cooling down or warming up?

The differences are usually **less than 3%** when testing the same temperatures.

## 2. Does temperature reach equilibrium between the inner and outer walls of the calibration housing?



Uncertainties range from **1% - 6%**, when the number concentration of water vapor molecules range from  $1.51e+17$  to  $2.09e+14$  #molec/cm<sup>3</sup>, respectively.

A **maximum  $\pm 6%$**  uncertainty when using this system at **0 to -65°C**.

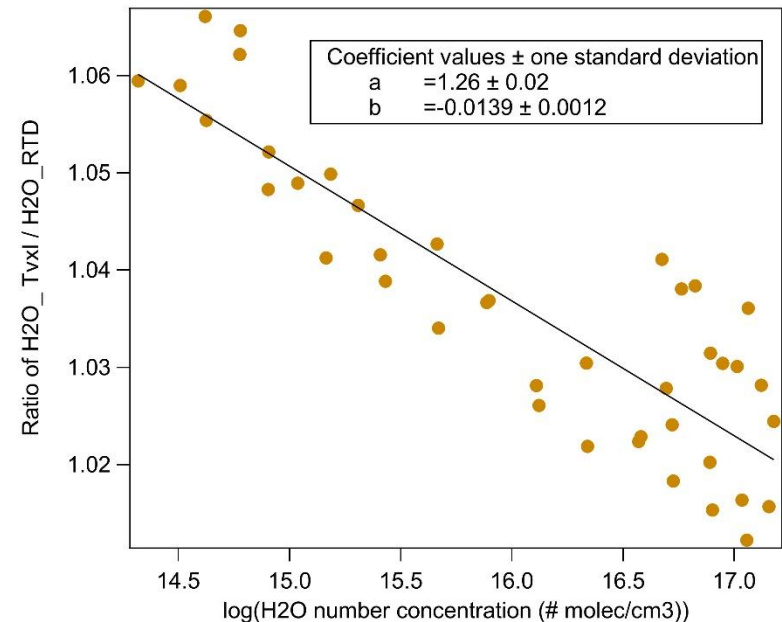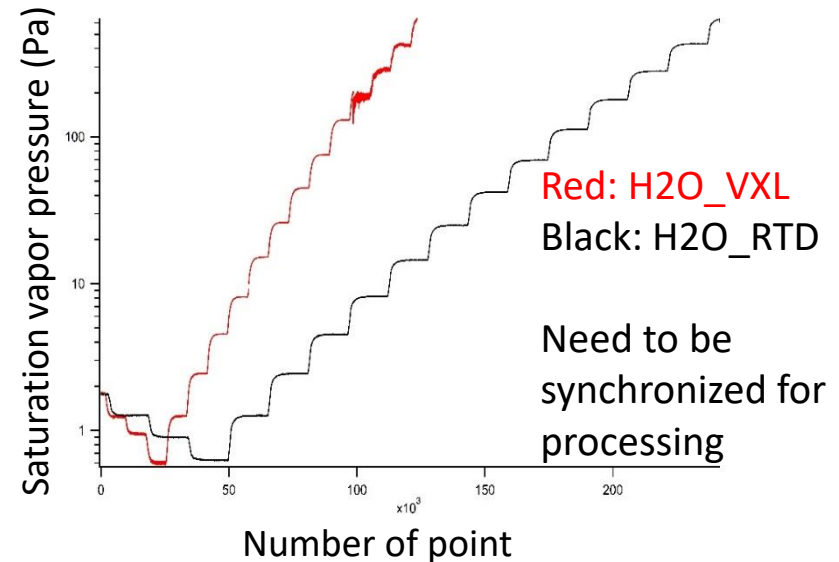



# Comparison of H<sub>2</sub>O from VCSEL and derived H<sub>2</sub>O from RTD

## (1) H<sub>2</sub>O\_VXL (v.2013.Princeton) vs H<sub>2</sub>O\_RTD temperature probe

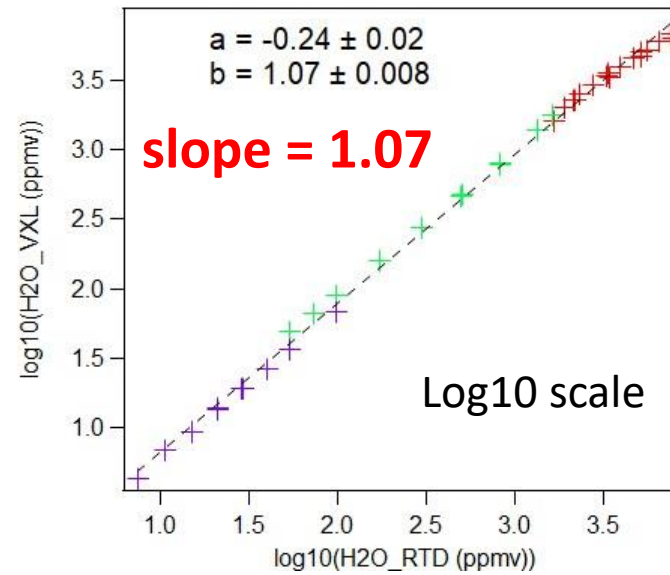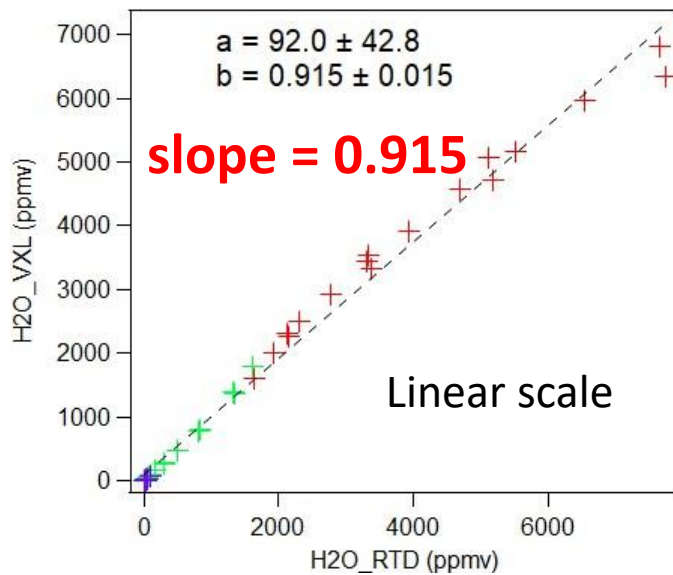


Red: weak mode  
Green: direct mode  
Purple: strong mode

## (2) H<sub>2</sub>O\_Temp\_vxl vs H<sub>2</sub>O\_RTD temperature probe

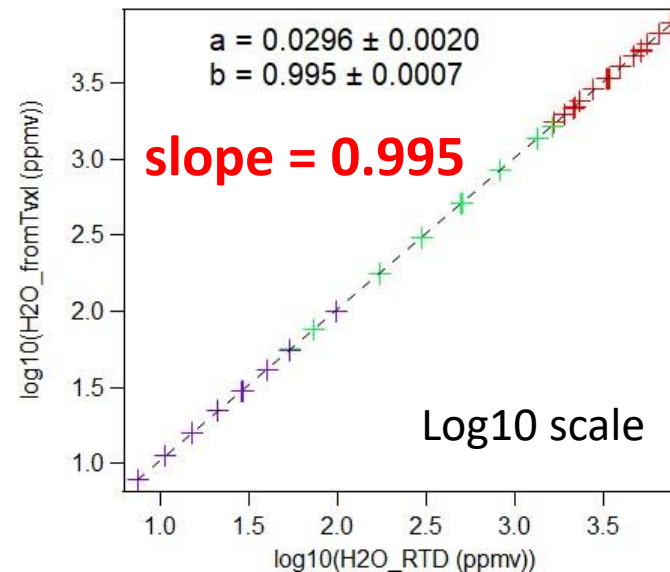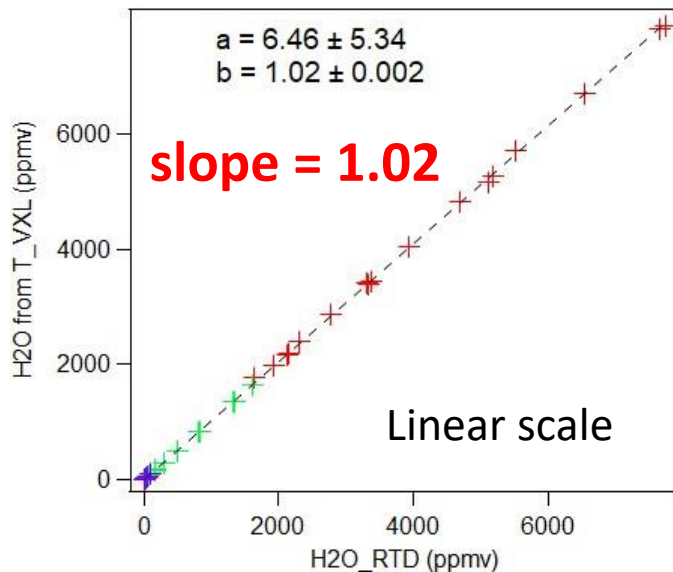


# Calibration equations of three modes for the VCSEL hygrometer


## Weak mode (Linear fit)

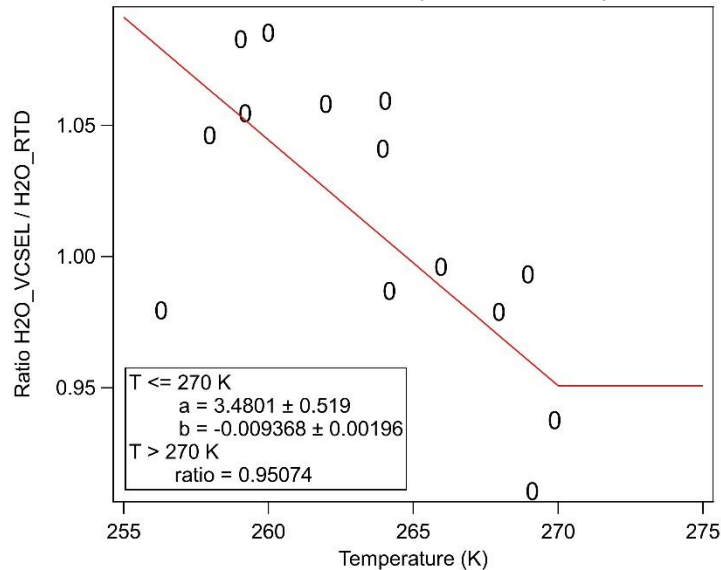

## Direct mode (Poly-3 fit)


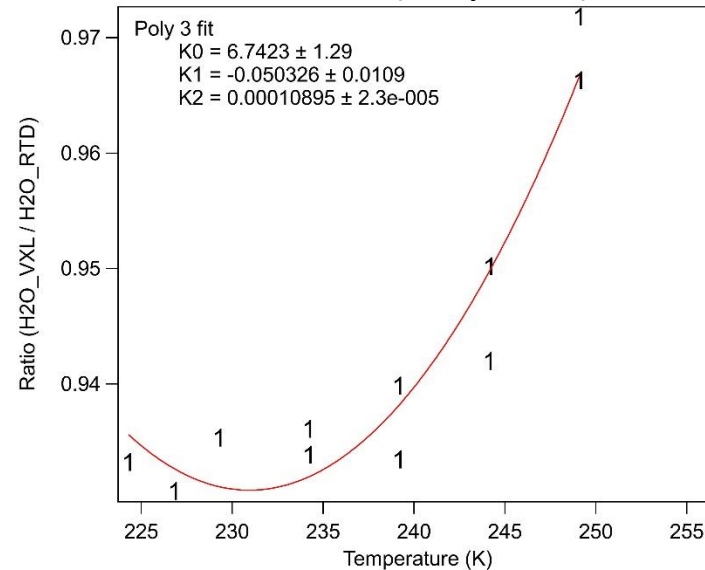


## Strong mode (Linear fit)

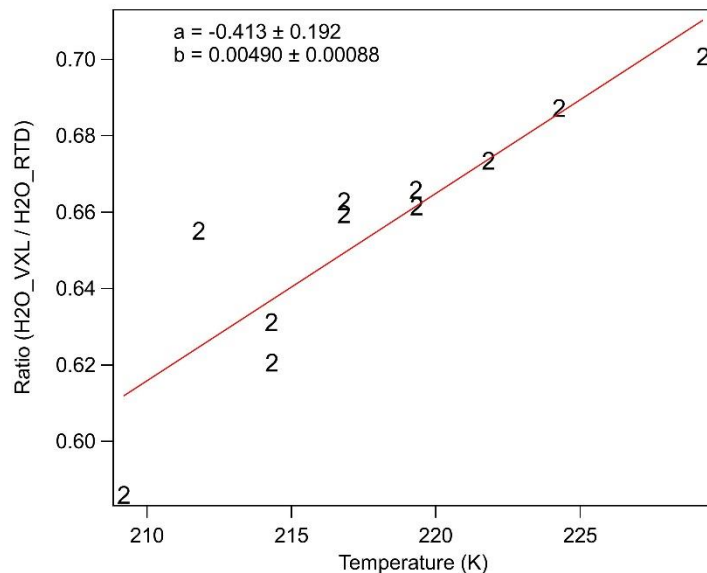


1. Regressions of ratio of H2O\_VXL / H2O\_RTD versus temperature (K)
2. Each mode has its own calibration
3. New water vapor data (**version.2018.1.Diao**) are calculated by applying the adjustments to the current water vapor data (**version.2013.Princeton**)

# Comparisons of the calibrated (v.2018.1.Diao) and current water vapor data (v.2013.Princeton)

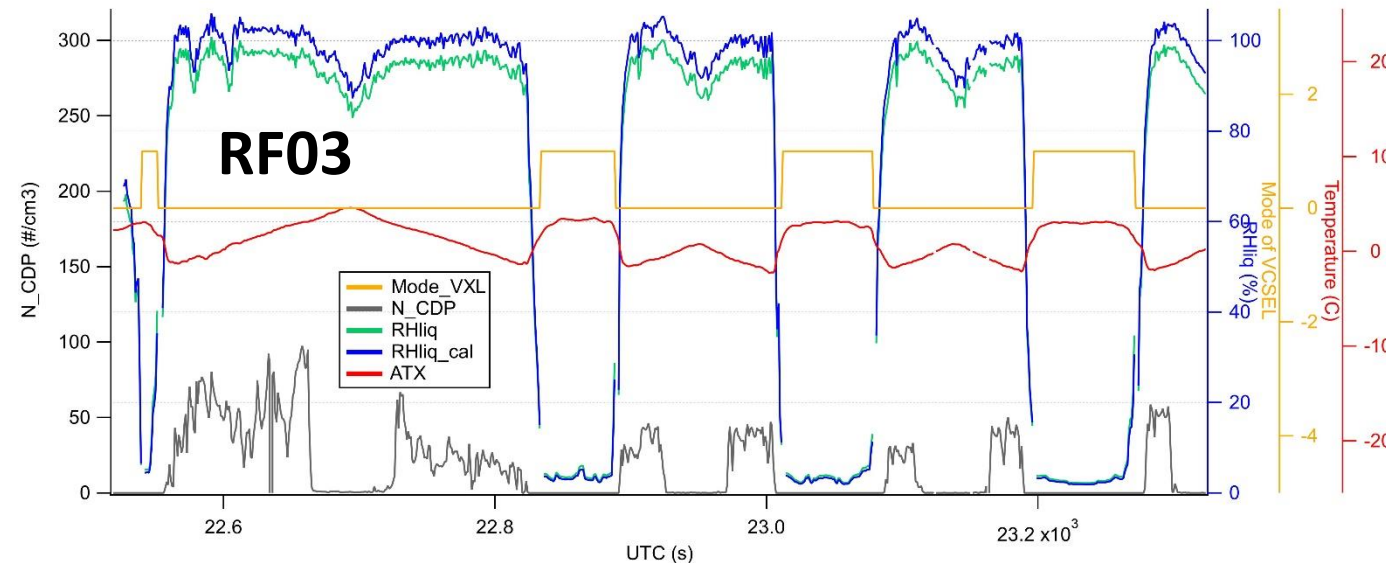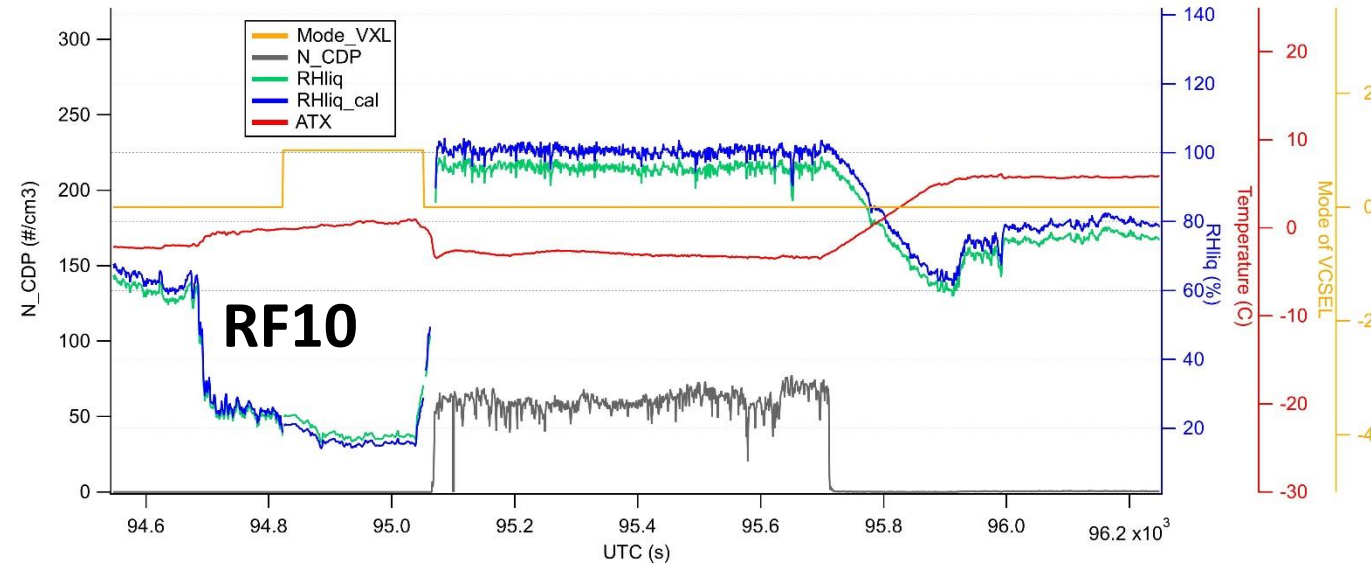


1. Water vapor data are generally adjusted to be **higher** at warmer temperatures
2. Most of the in-cloud conditions at warmer T show **liquid saturation** with v.2018.1.Diao
3. For cumulus sampling, **good synchronization** between RHliq and CDP number concentration

# Other examples of improvements with the calibration

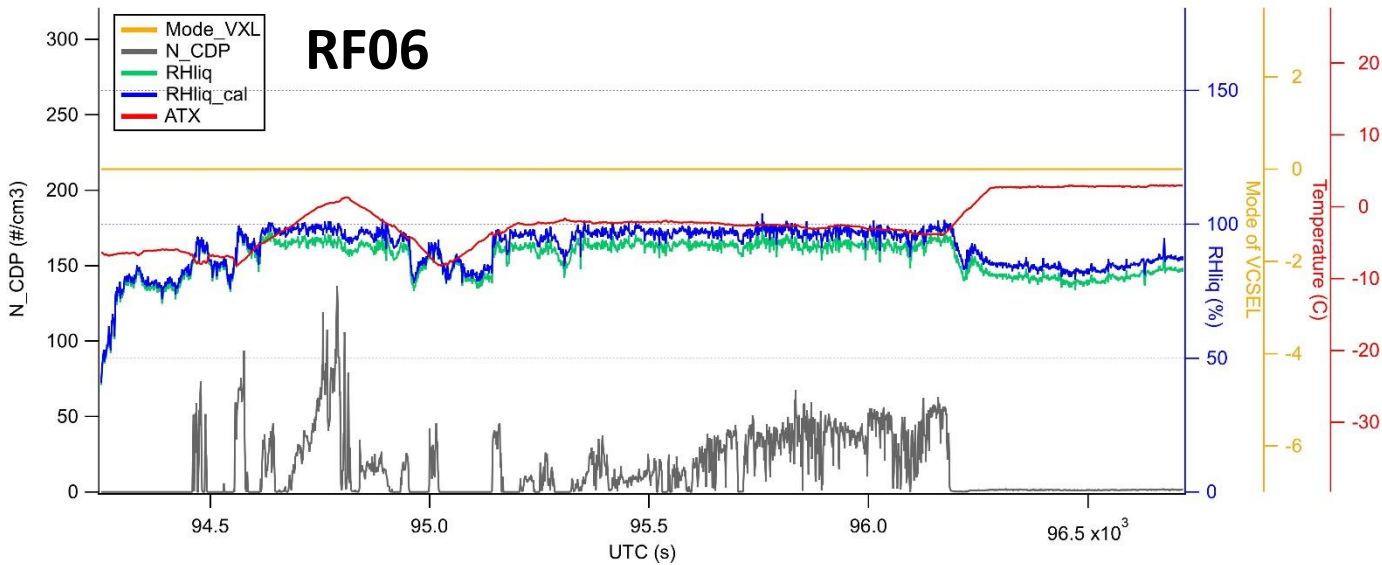





**RF06:** in-cloud leg around  $-5^{\circ}\text{C}$  is adjusted to be higher, reaching liquid saturation after calibration

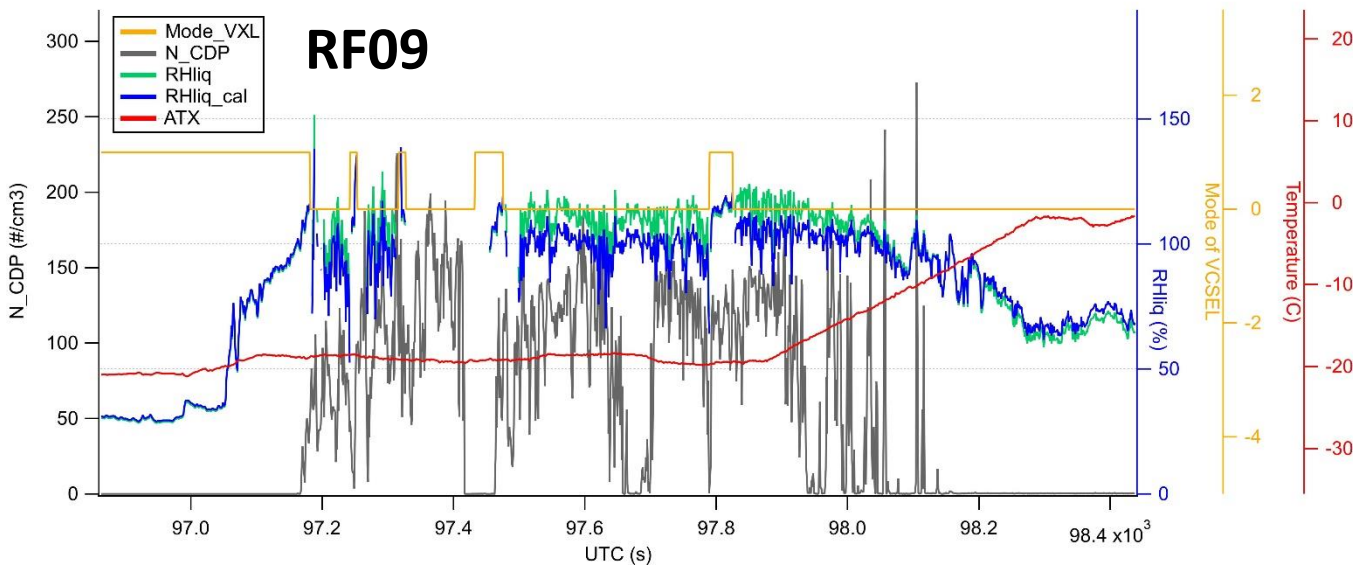

**RF09:** in-cloud leg around  $-20^{\circ}\text{C}$  is adjusted to be lower, closer to liquid saturation after calibration



# Relative humidity frequency distribution for in-cloud conditions at temperature $> -15^{\circ}\text{C}$

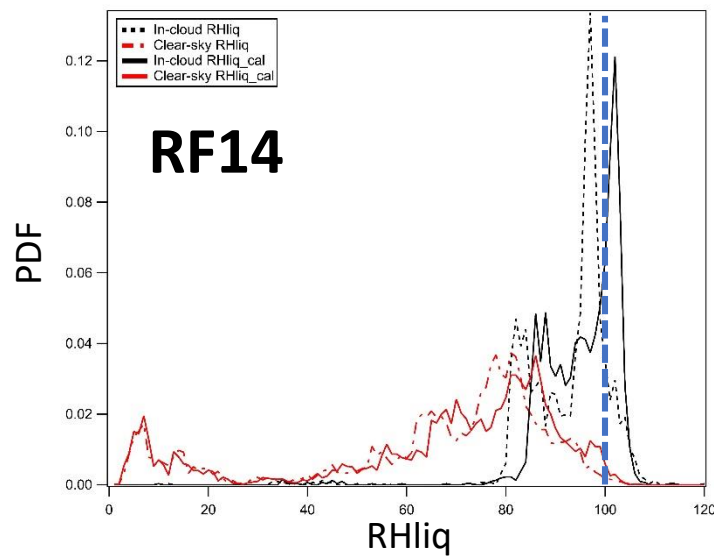
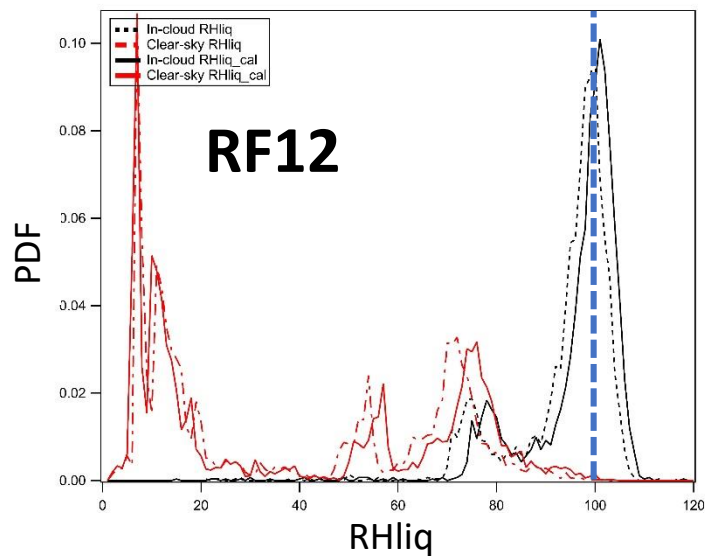
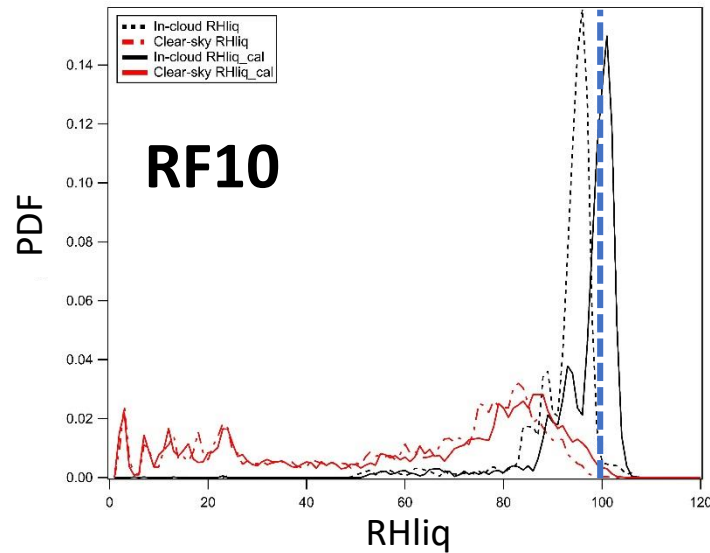
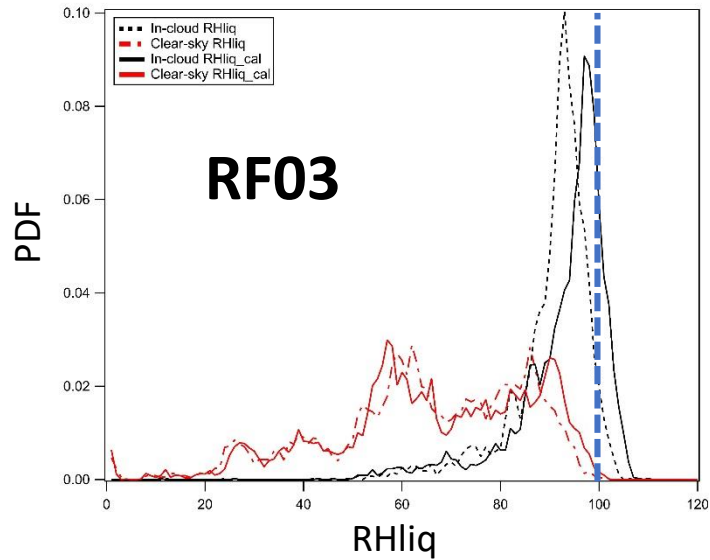


In-cloud:  
CDP  $> 1 \text{ cm}^{-3}$   
or, Fast-2DC  $> 0 \text{ L}^{-1}$

# SOCRATES RF10: RH distribution in different cloud phases

at  $-40^{\circ}\text{C} < T \leq 0^{\circ}\text{C}$

Diao and Yang (SJSU)

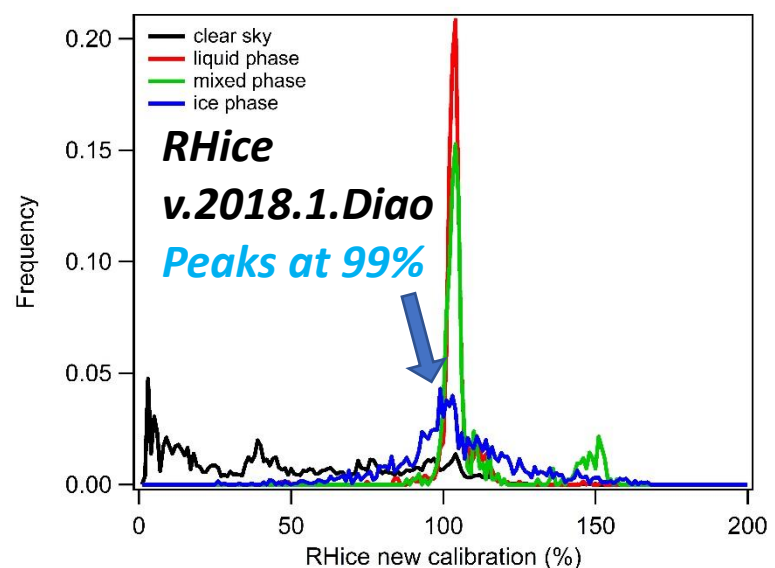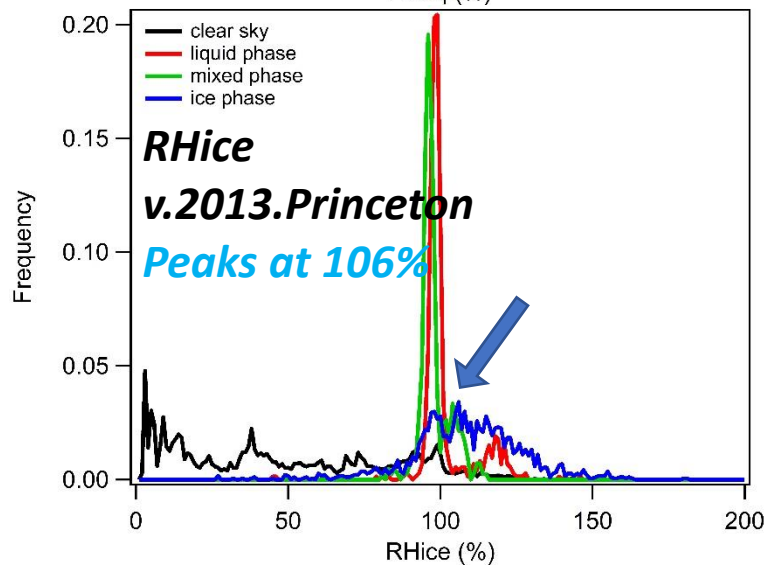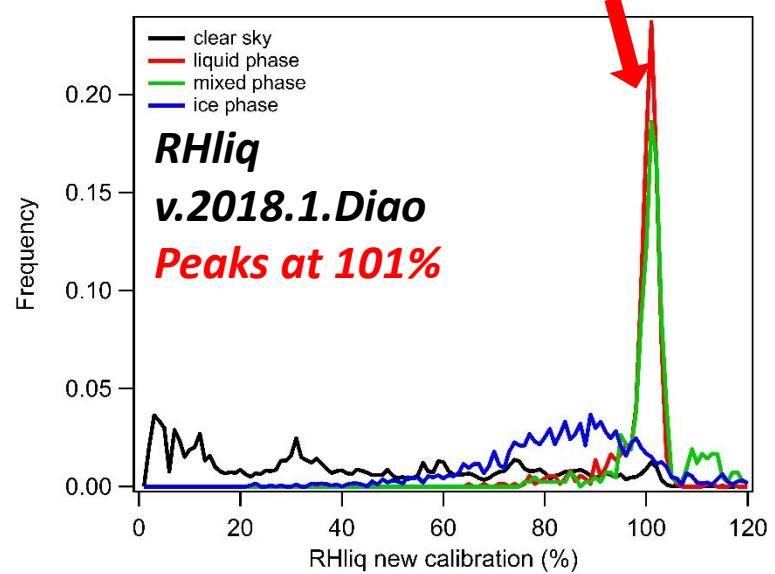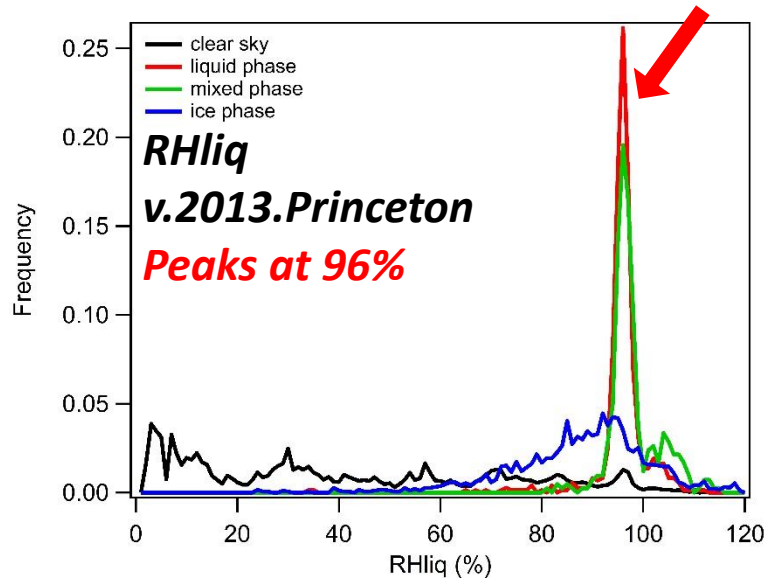

**Cloud phase id method:** D'Alessandro, J., M. Diao, C. Wu, X. Liu, B. Stephens, and J.B. Jensen, "Cloud phase and relative humidity distribution over the Southern Ocean based on in-situ observations and global climate model simulations", *Journal of Climate*, in revision.


# Summary of new calibration (v.2018.1.Diao)

1. Only temperature is considered as the factor; Overall, the calibration **improves** the statistical distributions of RHliq

2. Calibrated water vapor data (v.2018.1.Diao)

- increase H<sub>2</sub>O mixing ratio at  $T > 265$  K
- decrease H<sub>2</sub>O mixing ratio at  $255 \text{ K} < T \leq 265$  K
- Increase H<sub>2</sub>O mixing ratio at  $225 \text{ K} < T \leq 255$  K
- Increase H<sub>2</sub>O mixing ratio at  $210 \text{ K} < T \leq 225$  K

3. Table of individual peaks of in-cloud RHliq PDF (temperature  $> -15^\circ\text{C}$ )

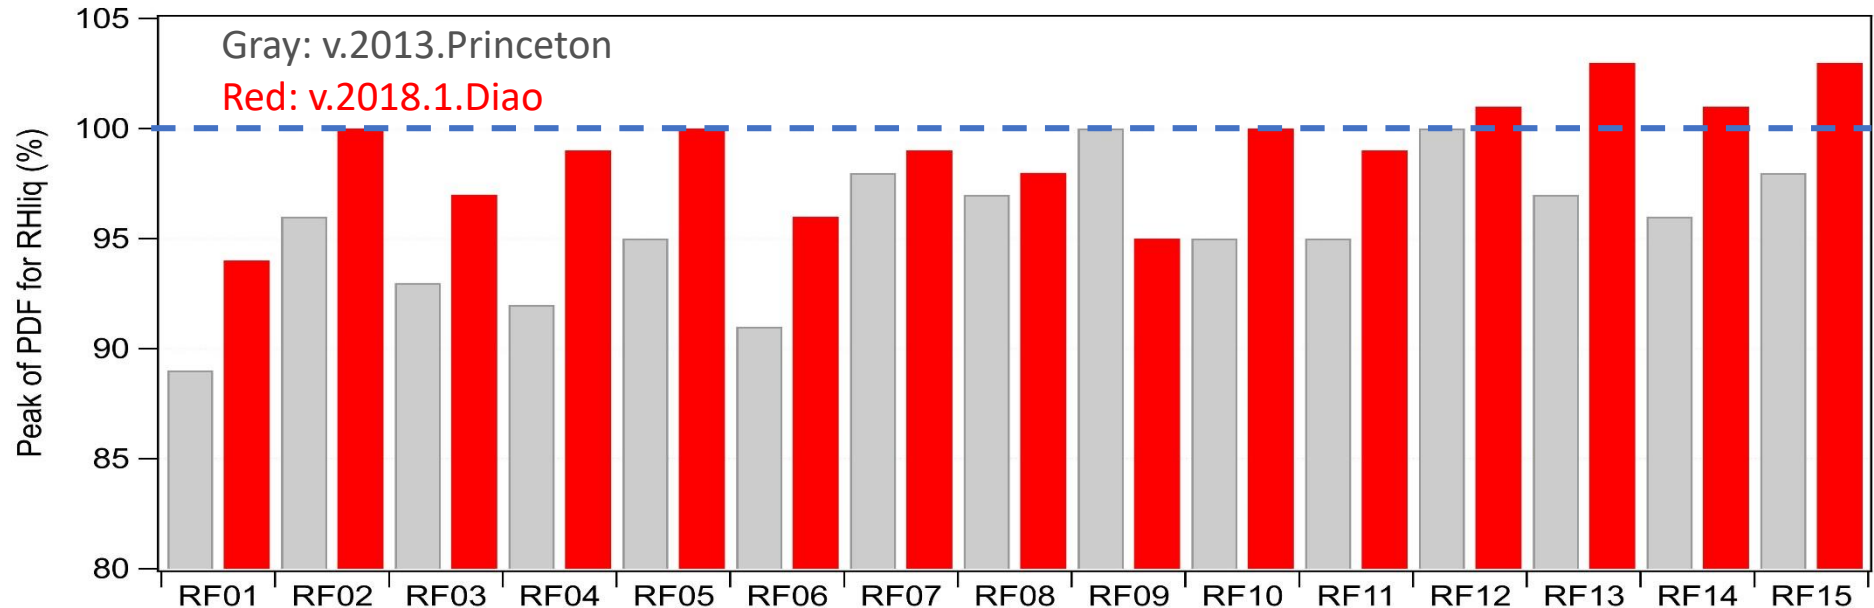

# Future work

- **Factors that remain to be addressed**
  - pressure
  - water vapor (sub-saturated conditions)
  - laser intensity
- **Use a different calibration system** – test the Princeton calibration chamber
- **Use additional water vapor source** - add a dewpoint generator for even warmer temperatures ( $> 0^{\circ}\text{C}$ )
- **Hysteresis when switching modes** – more time series focusing on transitions

## Acknowledgement

1. NCAR Advanced Study Program Faculty Fellowship 2018 and 2016
2. NSF Office of Polar Program grant #1744965
3. Thanks to EOL and RAF scientists for hosting my group in the summer of 2018 and 2016.
4. Many thanks to **Stuart Beaton** and **Laura Tudor** for setting up the laboratory experiments

